


# miniVNA-pro - 190804\_023300

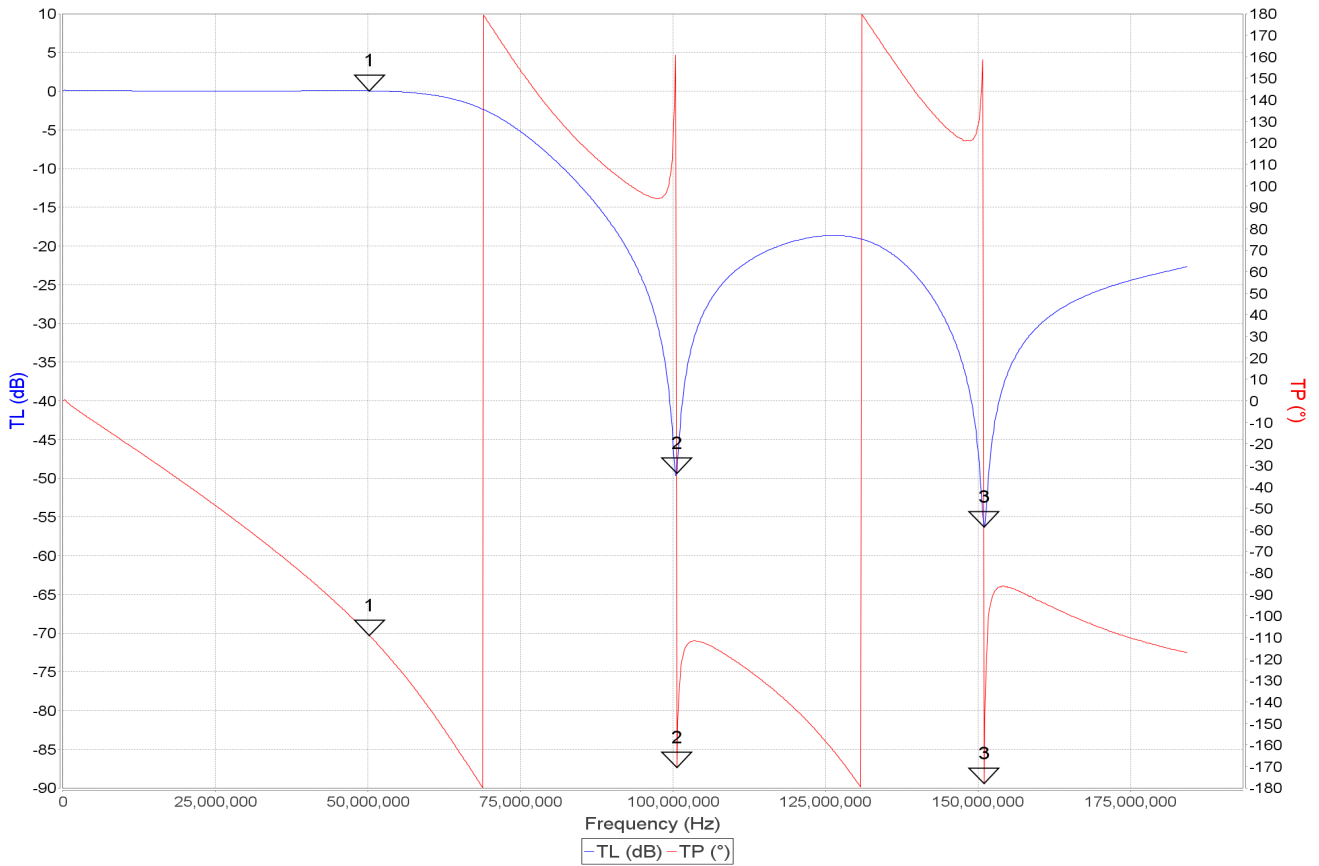

Marker	Freq. (Hz)	TL (dB)	TP (°)	Z  (Ω)	Rs (Ω)	Xs (Ω)	Theta	gr (ns)
1	50,256,652	0.04	-109.18	115.6	-67.3	-94.1	0.0	8.1
2	100,595,031	-49.40	-170.55	29398.8	28997.5	-4840.9	0.0	-440.5
1-2	50,338,379	49.43	61.38	29283.1	29064.8	4746.8	0.0	---
3	150,933,410	-56.31	-178.11	65295.7	65259.9	-2160.3	0.0	-354.2

## Comment:

Date: 8/4/19 2:33 AM  
 Mode: Transmission  
 Analyser: miniVNA-pro / mini radio solutions - miniVNA pro  
 Scan  
   Start: 100000 / 100,000  
   Stop: 199999960 / 199,999,960  
   Samples: 1014  
   Overscan: ?  
 Calibration  
   Samples: 1000  
   Overscan: 0  
   File: TRAN\_miniVNA-pro\_trans.cal  
 User: IGE  
 Headline: {2} - {0,date,yyMMdd}\_{0,time,HHmmss}  
 Port extension len: <not set>m

Port extension vf: <not set>